



MODEL 6800T COMPACT DRY QHR SYSTEM

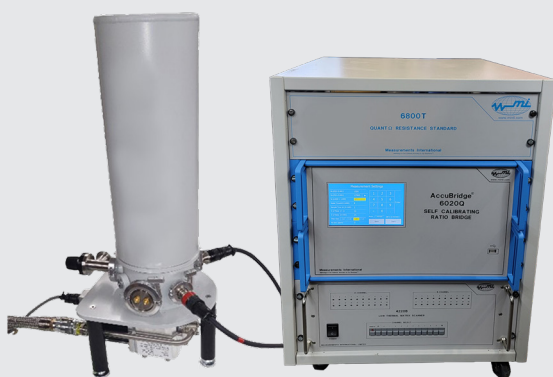


Figure 1
*Option shown 6800T-6020Q-4210B

6800T

- Cryogen-Free Dry System
- System Accuracy to < 0.003 ppm with CCC Model 6200A
- System Accuracy to < 0.015 ppm with DCC Model 6020Q
- 5 Tesla Standard System Magnet
- Stable Controlled Sample Environment
- Base Temperature < 3.6 K
- Low Operating Costs
- Direct Transfer to 100Ω , $1 \text{ k}\Omega$, $10 \text{ k}\Omega$, and 100Ω Standards
- System Range 0.1Ω to $100 \text{ k}\Omega$
- Graphene Device values $1 \text{ k}\Omega$, $10 \text{ k}\Omega$, $12.9064037 \text{ k}\Omega$ and $100 \text{ k}\Omega$
- Triple Sample Device Mounting

Introducing the Revolutionary MI 6800T QHR System: Your New Intrinsic Resistance Standard in today's rapidly evolving world, precision and accuracy are paramount, National laboratories and industries around the globe demand reliable, traceable reference standards to ensure the integrity of their measurements. That's where Measurements International (MI) steps in with the measurement-changing 6800T QHR Table Top System.

Let's talk about efficiency. With the 6800T, you can say goodbye to the headaches of liquid helium shortages, unpredictable deliveries, and skyrocketing prices. These challenges have become all too common, impeding the progress of countless labs. The 6800T requires no liquid helium to operate, ensuring uninterrupted and cost-effective performance. Drawing upon years of expertise in Quantized Hall System design, resistance measurements, and cryogenics, the MI 6800T is a fully automated primary standard. It has been meticulously engineered to deliver highly reproducible resistance standards, empowering you to achieve your measurement goals with ease. The system has a modular design, consisting of three essential components: the QHE samples, cryogenics system, and bridge measurement system. This seamless integration guarantees a streamlined workflow and allows for effortless customization to suit your specific requirements. Each component can be ordered individually to meet your laboratory needs and requirements.

The MI 6800T QHR System is backed by our unwavering commitment to customer satisfaction. We provide comprehensive support, ensuring a smooth installation process, extensive training, and ongoing assistance whenever you need it. With us by your side, you can focus on what matters most – advancing your research and calibration, and exceeding your performance targets.

Metrology is Our Science, Accuracy is Our Business™



Cryogenics and Magnet System

The 6800T offers customers ultra-reliable and high-performance range of cryogen-free magnet systems with sample space temperature of 3.6 K, and magnetic fields up to 5 Tesla in our standard system – all without the need for liquid cryogenes. Reliable, precise and highly stable temperature control is achieved during normal measurement sequences. Once connected to mains power these systems can be turned on and operational within several hours. With service intervals $\geq 30,000$ hours, the system may be used continuously over very long periods, or simply as needed, providing complete freedom to plan research work and optimize running costs.

Operation of the cryogenics is simple and easy to use. Once system is evacuated and ready for cooldown, simply turn on the compressor and wait for the temperature to drop to operation value. Typical cooldown time is under 7 hours. Once cold the system can run 24 hours a day, 7 days a week without intervention.

Magnet Specifications

| Superconducting Magnet | |
|---------------------------------|---|
| Magnet Type | Solenoid |
| Rated Central Field | 5.0 T |
| Rated Operating Current @ 6.0 T | 25.45 A |
| Total Inductance | 10.526 H |
| Homogeneity | $\pm 0.2\%$ 1 cm DSV |
| Superconductor | Twisted Multi-filamentary NbTi/Cu |
| Fabrication | Wet wound with epoxy to prevent training |
| Quench Protection | Adiabatic protection using copper matrix and diodes |


Example Magnet Specifications

| | |
|-------------------------------------|-----------------------------|
| Rated Central Field* | 5.0 T |
| Maximum Test Field | 5.0 T |
| Measured Current at 6.0 T | 25.45 A |
| Inductance | 11.03 H |
| Field-to-Current Ratio | 2357.5 G/A |
| Charging Rates | 0.0901 A/s (1.0V) 0-25.45 A |
| Persistent Switch Heater Current | NA |
| Persistent Switch Heater Resistance | NA |
| Magnet Resistance (at input leads) | 1.9 k Ω |
| System Cooldown Time | 7 hours |
| Cryogenics System Weight | 67.3 lbs |

Example Magnet Specifications



System Cooldown

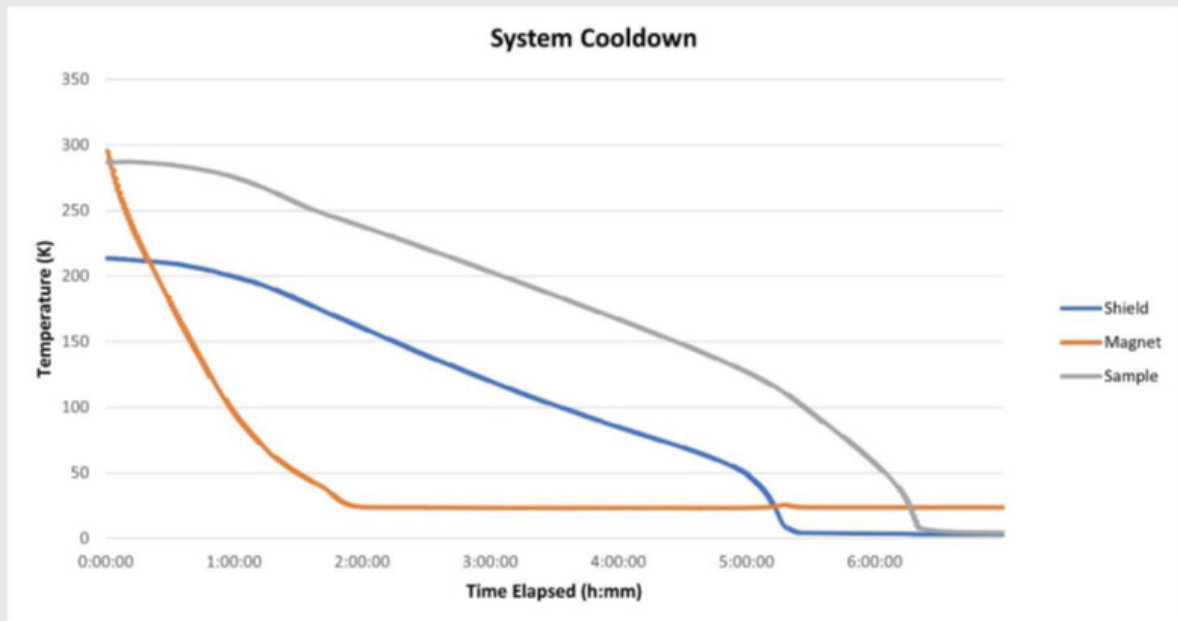

Cryocooler Specifications

| Cryocooler | |
|-------------------------|--|
| Cooling Powers at 50 Hz | 1st Stage: 35 W @ 45 K 2nd Stage: 0.9 W @ 4.2 K |
| Base Temperature | < 3.6 K |
| Orientation | Vertical Only |
| Maintenance Interval | 30,000 hrs - 40,000 hrs |
| Ambient Temperature | 5 °C to 35 °C |




| Compressor - F70LP/H (Water Cooled) | |
|-------------------------------------|---|
| Main Power Requirement | 7.2 kW (steady), 8.5 kW (max), 3-phase F70LP: 200 V @ 50 Hz & 60 Hz F70H: 380 - 415 V @ 50 Hz - 480 V @ 60 Hz |
| Water Cooling | 6.8 - 9 L/min |
| Ambient Temperature | 5 °C to 35 °C |
| Charcoal Absorber Life | 30,000 hrs |
| Flexible Gas Lines | 20 A x 20 m |
| Compressor Dimensions | W 444 mm, L 529 mm, H 576 mm |
| Weight | 100 kg |

Metrology is Our Science, Accuracy is Our Business™



QHE Devices

Measurements International has signed a partnership agreement with a world leading National Metrology Institute in the supply of Graphene Devices. The devices are fabricated with multiple values on each device providing not only the 12.9064037 k Ω value, but also offering QHARS values of 100 Ω , 1 k Ω , 10 k Ω and 100 k Ω . These values replace the need for air or oil resistors at those levels. Up to three devices can be mounted in the system.

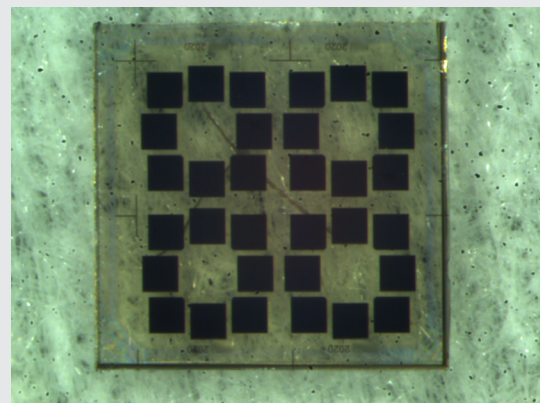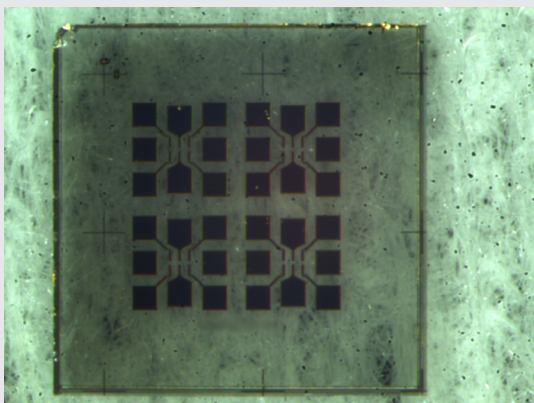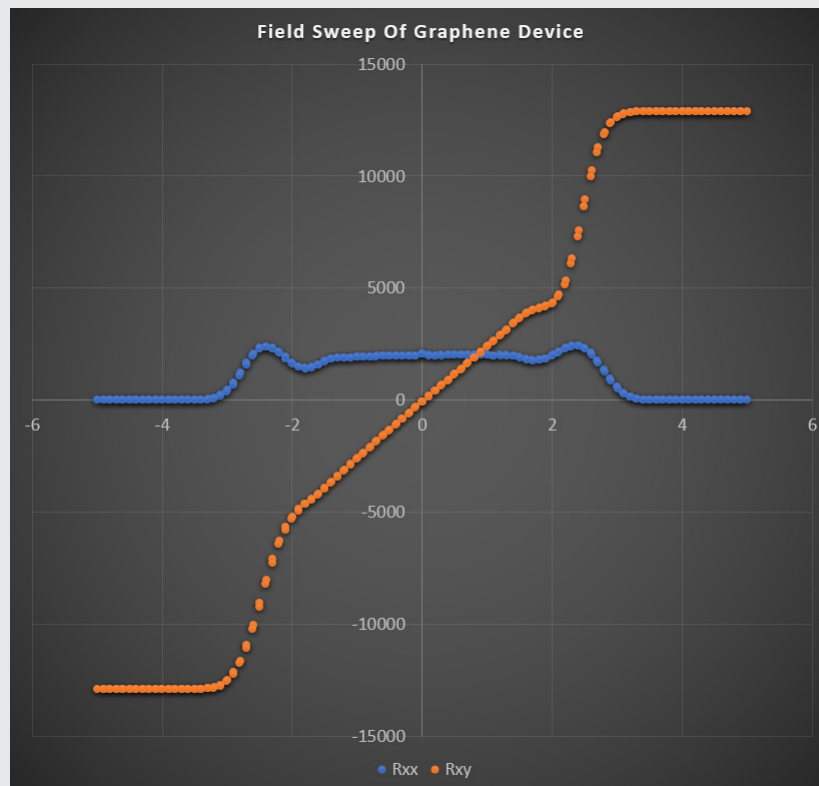

A QHARS device that contains a hall bar and 100 Ω , 1 k Ω , and 10 k Ω arrays

Metrology is Our Science, Accuracy is Our Business™



Measurements Bridges

The 6800T operates using either the 6200A Cryogenic Current Comparator system or the 6020Q room temperature DCC bridge, both offered by Measurements International. Both measurement bridges are simple, and easy to use.

For more information on the measurement bridges, visit <https://mintl.com/products/6200a-cryogenic-current-comparator-ccc/> and <https://mintl.com/productcategories/metrology/resistance-measurement/resistance-bridges/> or contact sales@mintl.com

Each system is offered with optional equipment like the MI 10-channel or 20-channel scanner allowing you full automation of scaling down to 0.1 Ω and up to 100 k Ω without the need for manual insurction when using the 6020Q.

Bridge Specifications

6200A

| Range (1:1 Ratio) | Accuracy ($\mu\Omega/\Omega$) | Range (1:10 Ratio) | Accuracy ($\mu\Omega/\Omega$) | Ratio (1:100 Ratio) | Accuracy ($\mu\Omega/\Omega$) |
|----------------------------------|---------------------------------|---------------------------------|---------------------------------|--------------------------------|---------------------------------|
| 0.1 Ω to 0.1 Ω | 0.01 | 0.1 Ω to 1 Ω | 0.01 | 1 Ω to 100 Ω | 0.003 |
| 1 Ω to 1 Ω | 0.003 | 1 Ω to 10 Ω | 0.003 | 100 Ω to 10 k Ω | 0.003 |
| 10 Ω to 10 Ω | 0.003 | 10 Ω to 100 Ω | 0.003 | 1 k Ω to 100 k Ω | 0.003 |
| 100 Ω to 100 Ω | 0.003 | 100 Ω to 1 k Ω | 0.003 | 10 k Ω to 1 M Ω | |
| 1 k Ω to 1 k Ω | 0.003 | 1 k Ω to 10 k Ω | 0.003 | | |
| 10 k Ω to 10 k Ω | 0.003 | 1 k Ω to 13 k Ω | 0.003 | | |
| 100 k Ω to 100 k Ω | 0.005 | 10 k Ω to 100 k Ω | 0.005 | | |
| 1 M Ω to 1 M Ω | 0.01 | 100 k Ω to 1 M Ω | 0.01 | | |

6020Q

| Note: Either R_s or R_x can be selected as the standard. 6020Q uncertainties in the bridge and software are specified at the 2σ level (95 %) this includes all secondary specifications such as linearity and noise with a ± 2 $^{\circ}\text{C}$ temperature variance. | 0.1 Ω to 100 k Ω | | | |
|---|--------------------------------|-------------------------|---------|---------|
| | R_x | Ratio & Accuracy (ppm)* | | |
| | - | 1:1 | 10:1 | 14:1 |
| | 0.1 Ω | < 0.02 | - | - |
| | 1 Ω | < 0.015 | < 0.015 | < 0.015 |
| | 10 Ω | < 0.015 | < 0.015 | < 0.015 |
| | 100 Ω | < 0.015 | < 0.015 | < 0.015 |
| | 1 k Ω | < 0.015 | < 0.015 | < 0.015 |
| | 10 k Ω | < 0.02 | < 0.015 | - |
| | 100 k Ω | - | < 0.05 | - |



Ordering Information

Each item can be ordered individually or as a system

| Item | Description |
|--------|---|
| 6800T | Table Top QHR System |
| 6200A | Cryogenic Current Comparator Bridge |
| 6020Q | DCC Resistance Ratio Bridge |
| QHR_01 | Graphene Device 12.9 k Ω |
| QHR_02 | Graphene Device 12.9 k Ω , 100 Ω |
| QHR_03 | Graphene Device 12.9 k Ω , 100 Ω , 1 k Ω , 10 k Ω |
| QHR_04 | Graphene Device 12.9 k Ω , 1 k Ω , 10 k Ω , 100 k Ω |


Options

| Item | Description |
|---------------|---|
| Chiller | Water Chiller Required if Suitable Cold Water Supply is Not Available |
| 4210A | 10-Channel Matrix Scanner |
| 4220A | 20-Channel Matrix Scanner |
| 9300 | 50 mK Temperature Controlled Air Bath - 50 Litres |
| 9300A | 15 mK Temperature Controlled Air Bath - 106 Litres |
| 9400 | 2 mK Temperature Controlled Oil Bath |
| 9210A/1 | Evanohm Resistor (1 Ω and 0.1 Ω) |
| 9210B | Oil Resistors 10 Ω , 100 Ω , 1 k Ω , 10 k Ω , 100 k Ω |
| 9331R | Air Resistors 1 Ω , 10 Ω , 100 Ω , 1 k Ω , 10 k Ω , 100 k Ω |
| SPSCW30/100 | 4-Conductor Teflon Cable, 30 m or 100 m |
| 6020Q-NMI-Cal | 6020Q NMI Calibration 5 Points |


How to Order:

Full System order includes selections from A+B+C


Items can also be ordered individually




A
Cryogenics



B
Measuring Bridge



C
QHR Device



D
Additional Items